

Change of Nano Material Electrical Characteristics for Medical System Applications [Corrigendum]

Chen P, Zhang X, Jiang K, et al. *Int J Nanomedicine*. 2019;14:10119–10122.

Page 10120, left column, Materials And Methods section, line 2, the text “30 ~ 50 nm thick” should read “30 ~ 60 nm thick”.

Page 10120, Figure 2, the Y axis “ $I_{DS}(nA)$ ” should read “ $I_{DS}(pA)$ ”.

Figure 3 on page 10120, the authors have advised the figure was created using the wrong sample and therefore, is incorrect. The correct Figure 3 is shown below.

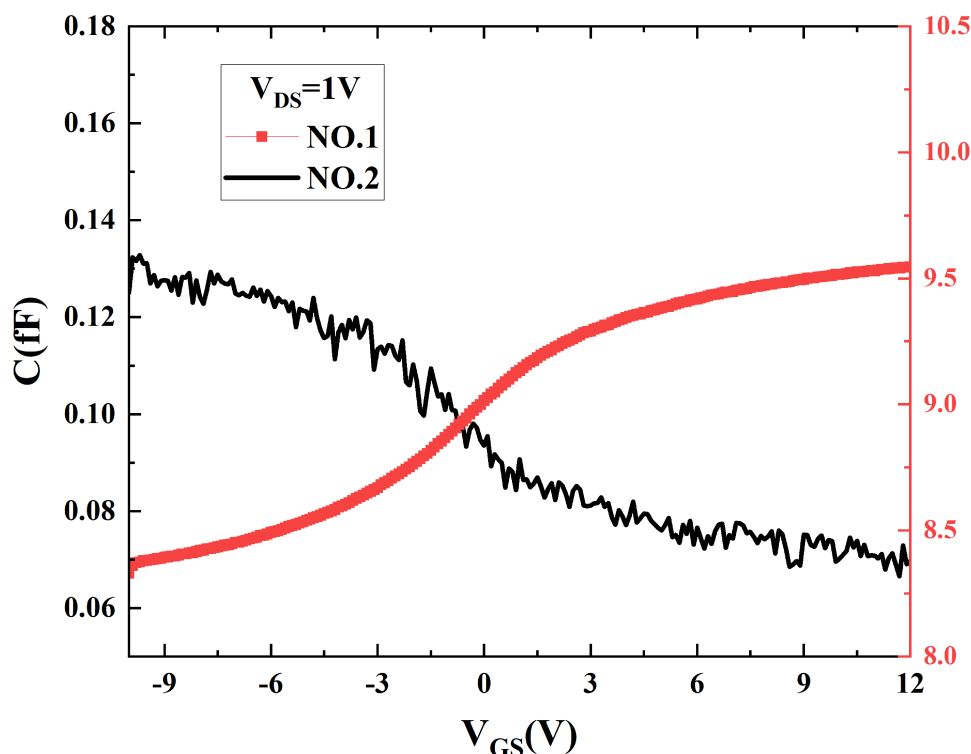


Figure 3 The C-V curve of the present n-type TFTs could be easily changed to that of p-type TFTs.

The authors apologize for these errors and advise they do not affect the results of the paper.

International Journal of Nanomedicine

Dovepress

Publish your work in this journal

The International Journal of Nanomedicine is an international, peer-reviewed journal focusing on the application of nanotechnology in diagnostics, therapeutics, and drug delivery systems throughout the biomedical field. This journal is indexed on PubMed Central, MedLine, CAS, SciSearch®, Current Contents®/Clinical Medicine, Journal Citation Reports/Science Edition, EMBase, Scopus and the Elsevier Bibliographic databases. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <https://www.dovepress.com/international-journal-of-nanomedicine-journal>

<https://doi.org/10.2147/IJN.S386292>